
# Spectrofluorometer

FP-8000 Series





Performance Innovation Reliability

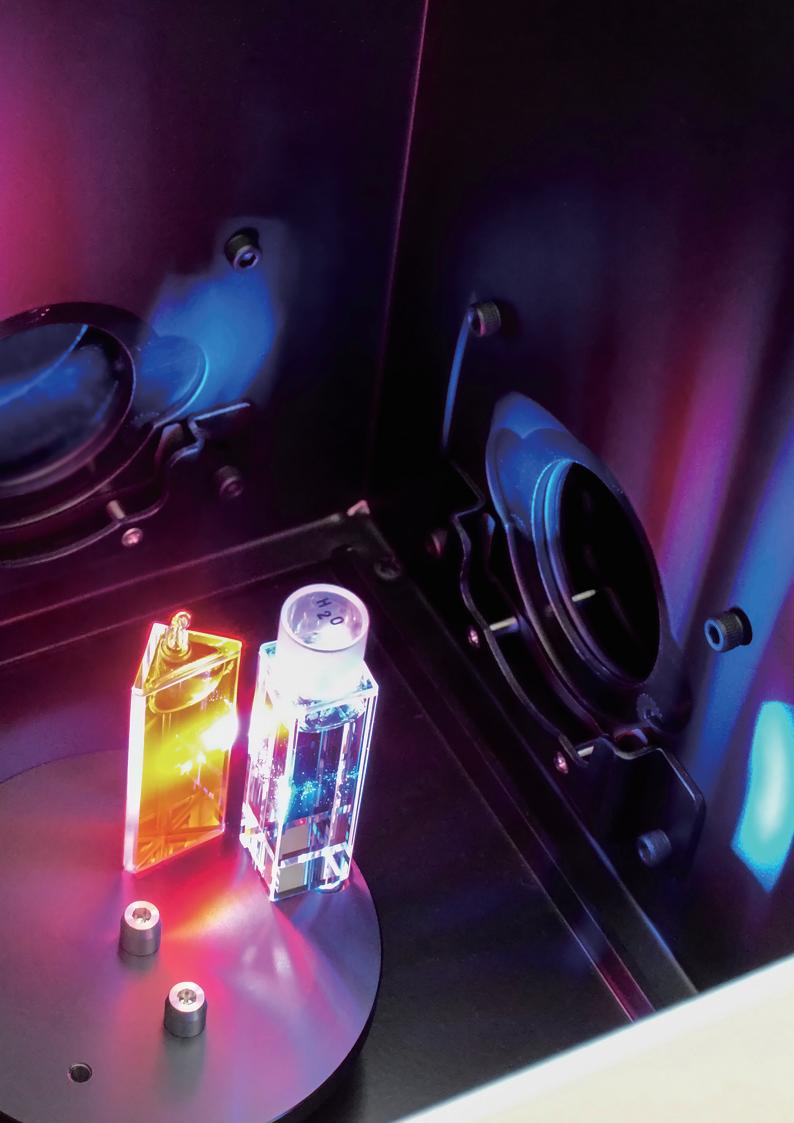

In 1967, JASCO launched the FP-1, which was the first in a long line of spectrofluorometers. The FP-8000 Series is the latest comprehensive range of instruments, developed to provide accurate measurements for bioand material sciences, from a simple entry level model for fluorescence spectral measurements and sensitive quantitation to the advanced models developed for demanding research applications including spectral correction and quantum yields.

The FP-8000 Series includes the powerful cross-platform Spectra Manager™ suite of software.

## Table of Contents

#### Instrument and Systems

| Instrument Features           | 4  |
|-------------------------------|----|
| Instrument Performance        | 8  |
| Accessories and Applications  |    |
| Accessories and Applications  | 10 |
| Software and Accessories      |    |
| Spectra Manager™              | 20 |
| Standard Measurement Programs | 22 |
| Optional Software             | 24 |
| iRM-900                       | 25 |
| Validation and Accessory Kits | 26 |
| Specifications                | 27 |
|                               |    |

# Features of the FP-8000 Series

For scientists performing biomolecule structure studies, advanced materials research, and quantum yield calculations who need confidence in the spectral purity of their measurements under a variety of conditions, the FP-8000 Series Spectrofluorometers provide an optical bench designed specifically for high sensitivity measurements with an expanded, wide dynamic range and automatic cut-off filters to exclude higher order diffraction.

The FP-8000 Series includes 5 different models with a large variety of accessories designed to meet your experimental needs.



#### **FP-8200**

The basic, compact model for routine measurements such as spectral scanning and quantitation.



#### FP-8300

Sophisticated optical system with additional features for biological applications.



#### FP-8500

The highest sensitivity and optimal spectral accuracy model with a wide range of accessories for maximum flexibility.



#### FP-8600

For extended wavelength operation into the near infrared.



#### FP-8700

With a liquid nitrogen PMT detector for applications that require high sensitivity measurements into the near infrared (1700 nm).

#### Advanced Features of the FP-8000 Series

- High throughput optical system
- Highest S/N performance
- Wide dynamic range (at least 6 orders of magnitude)
- Auto Gain and Auto Sensitivity Control System
- Automatic cut-off filters for higher-order diffraction
- High speed scanning
- Advanced digital signal processing
- Spectral Correction
- Spectral bandwidth down to 1 nm

#### **Unique Features and Accessories**

- Compact benchtop design
- Range of precise temperature control accessories
- Automatic polarizers to allow for automatic anisotropy measurements
- Quantum Yield Determination
- Automated Microplate Reader for rapid sample throughput
- Microsampling accessories for small volume samples
- Stopped-flow system allows for kinetic measurements
- Spectra Manager<sup>™</sup> software for control and data analysis
- Flexible design allows for field upgrades as measurement requirements change

#### Versatility for a Wide Range of Applications

- Protein dynamics
- Quantitative analysis
- Cellular membrane studies
- Enzyme kinetics
- Carbon nanostructures
- Fluorescent materials
- Short lifetime phosphorescence measurements

# FP-8500 Spectrofluorometer

## The FP-8500 has the highest sensitivity and optimal spectral accuracy with a wide range of accessories for maximum flexibility in experimental design.

The FP-8500 is a high performance spectrofluorometer with an optimized optical design for very low stray light and a dynamic range of up to 6.5 orders of magnitude. It is exceptionally sensitive with a water Raman S/N ratio of 8,500:1 (RMS), which allows for fast measurements of samples with low level fluorescence. The high spectral resolution of 1.0 nm, automatic cut-off filters for exclusion of higher-order diffraction, and accurate spectral correction assures accurate measurements for the evaluation of advanced materials. The high-speed scanning enables fast measurements of 3D spectra and phosphorescence samples.

The FP-8500 optical bench has been developed to take advantage of the wide range of sampling accessories and applications, such as temperature-dependence, anisotropy, FRET, spectral correction, and quantum yields.



#### Options

- Automatic polarizers
- Temperature control
- Stopped flow
- Integrating spheres
- Microplate Reader

- High sensitivity S/N 8,500:1 (RMS, water Raman)
- High-speed scanning up to 60,000 nm/min
- Wavelength range: 200 to 750 nm (850 nm optional)
- Validation accessory comes standard

# FP-8200 Spectrofluorometer

## A compact model for routine measurements such as spectral scanning, temperature dependent measurement and quantitation.

The FP-8200 is a general-purpose instrument. The simplified yet powerful design is perfect for users that require routine fluorescence measurements in a quality-control environment. The standard Auto-SCS and Auto-Gain features enable measurements to be obtained over a wide range of concentrations using only one method. Two graphical user interfaces are available: Spectra Manager<sup>™</sup> cross-platform spectroscopy software that allows full system control of the instrument, separate from the data processing and analysis, and the intelligent remote module (iRM) with a color LCD touch screen.



- High sensitivity S/N > 4,500 (RMS, water Raman)
- Dynamic range up to six digits
- High speed scanning up to 20,000 nm/min
- Wavelength range: 200 to 750 nm (900 nm optional)
- Higher order diffraction cut-off filter (optional)

# FP-8300 Spectrofluorometer

## Sophisticated optical system with additional features for biological applications.

The FP-8300 is a user friendly spectrofluorometer with a wide range of accessories that are well suited to biological research. The standard automatic cut-off filters obtain spectra without the artificial peaks due to second order diffracted light. The Auto-Gain and Auto-SCS functions optimize the S/N for samples with large differences in signal intensity and concentration. Temperature control accessories can be used for thermal melting studies, providing researchers with fluorescence and thermodynamic data for conformational and folding studies. FRET measurements offer insight on binding and folding dynamics. The FP-8300's automatic polarizers can perform fluorescence anisotropy measurements to provide information regarding fluorophore mobility. Kinetic and titration measurements can also be performed with the dedicated stopped-flow and autotitrator systems.



- High sensitivity S/N > 8,000:1 (RMS, water Raman)
- High resolution of 1.0 nm
- Wavelength range: 200 to 750 nm (900 nm optional)

# FP-8600 Spectrofluorometer

### For extended wavelength operation into the near infrared.

The FP-8600 spectrofluorometer uses a sensitive PMT to obtain data from the UV to the NIR regions. The excitation wavelength range of 200 to 850 and up to 1010 nm for fluorescence emission allows measurements of materials which have fluorescence in the NIR region, such as carbon nanotubes. The small instrument design incorporates high-speed scanning and automatic cut-off filters to exclude higher-order diffraction. The FP-8600 is also suitable for biological sample measurements when using an NIR fluorescence reagent to avoid auto-fluorescence.



- High sensitivity S/N > 3,500 (RMS, water Raman)
- High-speed scanning up to 120,000 nm/min Emission
- Wavelength range: 200 to 1010 nm Emission (850 nm, Excitation)
- Validation accessory as standard

# FP-8700 Spectrofluorometer

# With a liquid nitrogen PMT detector for applications that require high sensitivity measurements into the near infrared (1700 nm).

The FP-8700 includes a liquid  $N_2$  cooled PMT for enhanced sensitivity in the NIR region to 1400 nm (1700 as option).



- Liquid N<sub>2</sub> cooled PMT
- Excitation wavelength 200-850 nm
- Emission wavelength 300-1400 nm (1700 as option)
- Spectral correction
- Option for lower excitation

# Instrument Performance

## **Highest Sensitivity**


The high throughput optical system and low noise signal processing of the FP-8000 series provides users with a high S/N (signal-to-noise) performance of up to 8,500:1 (RMS). The advanced A/D converter enables rapid sampling and the high speed signal processing system that immediately converts the fluorescence signal from the detector to a digital signal without introducing any additional noise.

## Wide Dynamic Range

A wide dynamic range for luminescence measurements is obtained by using the Auto-Gain and Auto-SCS features, automatically adjusting the detector gain and sensitivity for optimum measurements.

## Auto-Gain


Auto-Gain automatically adjusts the gain of a signal from the detector, so that the S/N is optimized throughout the entire scan range for spectral or time course measurements. Since quantum yield measurements can produce peaks that vary greatly in fluorescence intensity, the auto-gain function assures the accuracy of the measurement.

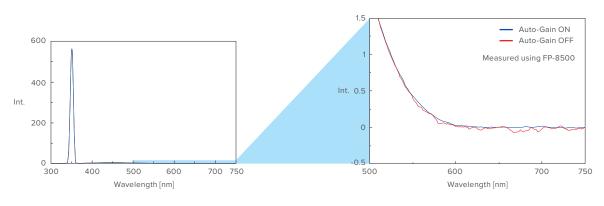




## Auto-SCS

The Auto Sensitivity Control System (SCS) allows users to create calibration curves for a wide concentration range without having to manually change the instrument Sensitivity settings. Auto-SCS can obtain measurements of sub-picomolar to micromolar concentrations for fixed wavelength measurements and quantitative analyses.

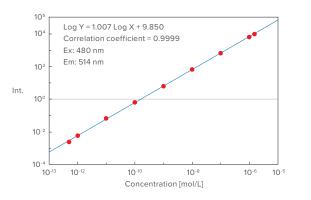

Calibration Curve of Fluorescein Solutions





## Automatic Cut-Off Filter for Higher-Order Diffraction


The new automatic cut-off filters remove peaks originating from higher-order diffracted light to provide simple and reliable spectral acquisition and analysis. The cut-off filters can also be used for spectral corrections, 3D measurements, and quantum yield determination.



3D Spectra of Fluorescent Orange Color Plate Left: Without Cut-Off Filter Right: With Cut-Off Filter

## **Spectral Correction**

JASCO has developed a spectral correction system to provide greater accuracy covering a larger wavelength range. While traditionally Rhodamine B was used for spectral correction of the excitation spectra, the use of calibrated deuterium and tungsten halogen Int. light sources and calibrated detector now provide corrected data which can be directly observed from the UV to NIR spectral regions.

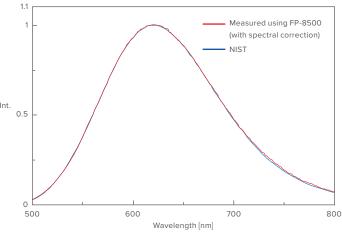

Spectra of NIST SRM-2940

#### Automatic Accessory Recognition

When an accessory is attached to the instrument sample compartment, Spectra Manager<sup>™</sup> automatically recognizes the installed accessory. Previously used instrument parameters associated with the accessory are recalled and information such as the accessory name and serial number are logged with the measurement file information. The IQ start system in conjunction with IQ Accessory recognition allows rapid access to pre-defined analysis methods.





# **Temperature Control**



ECH-813



ECH-815

## Single-Position Peltier Cell Holders

 EHC-813 | Air-Cooled Peltier Thermostatted Cell Holder with Stirrer

 ETC-814 | Water-Cooled Peltier Thermostatted Cell Holder with Stirrer

 ETC-815 | Water-Cooled Peltier Thermostatted Cell Holder with Stirrer

 Specifications

 Model
 EHC-813

 ETC-814
 ETC-815

| Model                        | EHC-813   | ETC-814 | ETC-815            |
|------------------------------|---|---------|--------------------|
| Compatible Cells             | Micro cell: 3x3 or 5x5 mm, Rectangular cell: 10x10 mm, 1 pc   |         |                    |
| Temperature Control System   | Heating/cooling system utilizing Peltier effect   |         |                    |
| Peltier Heat Radiation       | Air cooled Water cooled   |         |                    |
| Stirring System              | Integrated variable speed magnetic stirrer  |         |                    |
| Temperature Setting Range    | 5 to 70 °C -10 to 110 °C  |         |                    |
| Temperature Control Range    | 10 to 60 °C (at 25 °C) 0 to 100 °C (20 °C water temperature)  |         | water temperature) |
| Temperature Control Accuracy | ±0.1 °C   |         |                    |
| Temperature Accuracy         | With cell holder sensor: $\pm 0.5~^{\rm C}$ (20 to 40 $^{\circ}$ C), $\pm 1~^{\rm C}$ (<20 $^{\circ}$ C and >40 $^{\circ}$ C) With in-cell sensor: $\pm 0.2~^{\circ}$ C |         |                    |
| Standard Accessory           | In-cell sensor  |         |                    |

Multi-Position Peltier Cell Changer

#### PCT-818 | Water-Cooled Peltier Thermostatted 4-Position Automatic Cell Changer with Stirrer

| Specifications                          |   |  |  |  |
|---|---|--|--|--|
| Compatible Cells                        | Micro cell: 3x3 or 5x5 mm, Rectangular cell: 10x10 mm, 1 pc   |  |  |  |
| Temperature Control System              | Heating/cooling system utilizing Peltier effect   |  |  |  |
| Peltier Heat Radiation                  | Water cooled  |  |  |  |
| Stirring System                         | Integrated variable speed magnetic stirrer  |  |  |  |
| Temperature Setting Range -10 to 110 °C |   |  |  |  |
| Temperature Control Range               | 0 to 90 °C (at 25 °C)   |  |  |  |
| Temperature Control Accuracy            | ±0.1 °C (holder sensor)   |  |  |  |
| Temperature Accuracy                    | With cell holder sensor: ±0.5 °C (20 to 40 °C), ±1 °C (<20 °C and >40 °C)<br>With in-cell sensor: ±0.2 °C |  |  |  |
| Standard Accessory                      | In-cell sensor  |  |  |  |
| Optional Accessory                      | In-cell sensor, 3 piece set (factory option)  |  |  |  |
|   |   |  |  |  |



PCT-818

| used with all FP-8000 Series       | All Models   |
|------------------------------------|--------------|
| used only with FP-8200             | FP-8200      |
| used only with FP-8300             | FP-8300      |
| used only with FP-8500             | FP-8500      |
| used only with FP-8600 and FP-8700 | FP-8600/8700 |
| used only with Spectra Manager™    | PC           |
| purge is standard                  | Purge        |

## Constant Temperature Cell Holders/Changers

CTH-807 | Water Thermostatted Cell Holder

STR-811 | Water Thermostatted Cell Holder with Stirrer STR-812 | Water Thermostatted Cell Holder with Stirrer Specifications Model Name CTH-807 STR-811 STR-812 Compatible Cells Micro cell: 3x3 or 5x5 mm, Rectangular cell: 10x10 mm, 1 pc Temperature Control Thermostatted water circulation STR-811 Stirring System Integrated variable speed magnetic stirrer Operating Temperature 5 to 90 °C FCT-816 | Water Thermostatted Automatic 4-Position Turret Cell Changer FCT-816S | Water Thermostatted Automatic 4-Position Turret Cell Changer with Stirrer ( FCT-817 | Water Thermostatted Automatic 8-Position Turret Cell Changer ( FCT-817S | Water Thermostatted Automatic 8-Position Turret Cell Changer with Stirrer FCT-816 Specifications Model Name FCT-816 FCT-817 FCT-816S FCT-817S Compatible Cells Micro cell: 3x3 or 5x5 mm, Rectangular cell: 10x10 mm, 1 pc Temperature Control Thermostatted water circulation Stirring System Integrated variable speed magnetic stirrer Operating Temperature 5 to 90 °C CSP-828 | Sample Compartment Lid with Syringe Port CSP-829 | Sample Compartment Lid with Syringe Port Allows the addition of a reagent to the sample cell without opening and closing the sample compartment lid. It is recommended for use with cell holders that include an integrated stirrer, such as the STR-811/812, EHC-813 or ETC-814/815 cell holders. Compatible syringe needle: 2 inch (50 mm) CSP-829 \*3 mm microcell cannot be used. Other Temperature Control Accessories CTU-100 | Mini Water Circulation Bath

#### Specifications

| ·                           |   |  |  |
|-----------------------------|---|--|--|
| Dimensions                  | 170 (W) × 200 (H) × 311 (D) mm                                  |  |  |
| Temperature Control Range   | 10 °C below ambient temperature to 40 °C (IN and OUT connected) |  |  |
| Temperature Sensor Accuracy | ±0.2 °C (at 20 °C)  |  |  |
| Bath Capacity               | 100 mL  |  |  |
| Cooling/Heating Capacity    | 57 W  |  |  |



CTU-100

# Sample Holders

## Ambient Temperature Cell Holders

FUV-803 | Absorbance Measurement Cell Holder

#### Specifications

Wavelength Range

FHM-804 | High Sensitivity Measurement Cell Holder

The FHM-804 includes a reflection mirror used to improve light collection efficiency to increase the sensitivity of the fluorescence measurement.

220 to 900 nm; depending on configuration

#### FSA-805 | 30 Degree Incident Angle Cell Holder for Triangle Cell

#### FSA-806 | 30 Degree Incident Angle Cell Holder for Rectangular Cell

Specifications

| Model                    | FHM-804   | FUV-803                       | FSA-805         | FSA-806                       |
|--------------------------|---|-------------------------------|-----------------|-------------------------------|
| Compatible Cells         | Micro cell: 3x3 or 5x5<br>mm, Rectangular cell:<br>10x10 mm                     | Rectangular cell:<br>10x10 mm | Triangular cell | Rectangular cell:<br>10x10 mm |
| Diffusion Plate Material |   | Spectralon                    |                 |                               |
| Sensitivity              | Max 3x higher than<br>standard cell holder<br>(0.05 Abs or less,<br>10 mm cell) |                               |                 |                               |





FHM-804



FSA-805

## Solid Sample Holders

The FDA-808 is used for solid and powder samples, the FLH-809 is used for films and solid samples, and the FPA-810 is dedicated to powder sample measurements and can also be used for micro powder samples.

FDA-808 | Solid Sample Holder







PSH-002



FLH-809

PSH-102



FPA-810 | Powder Sample Cell Holder

FDA-808

PSH-103

FPA-810

| Specifications       |                  |   |                    |                               |
|----------------------|------------------|---|--------------------|-------------------------------|
| Model Incident Angle |                  | FDA-808                                 | FLH-809            | FPA-810                       |
|                      |                  | 30 deg.                                 |                    |                               |
| Min sample size      |                  | 25 (H) x 25 (W) mm                      | 12 (H) x 12 (W) mm | _                             |
| Solid Sample         | Max sample size  | 50 (H) x 50 (W) mm                      | 50 (H) x 50 (W) mm | _                             |
|                      | Sample thickness | 10 mm or less                           | 18 mm or less      | _                             |
| Devider Comple       | Standard cell    | FP-1061 Powder sample cell              | -                  | PSH-101 Powder sample cell    |
| Powder Sample        | Cell holder size | φ 20.5 mm, thickness 1 mm (with spacer) | _                  | φ 12 mm, thickness 0.5 - 4 mm |

#### PSH-002/102/103 | Optional Cells for FPA-810

Specifications

| Model      | PSH-002     | PSH-102 | PSH-103 |
|------------|-------------|---------|---------|
| Cell Size: | φ 16 mm     | ф 8 mm  | φ 5 mm  |
| Thickness: | 0.5 to 4 mm |         |         |

#### 250BP30 | Optional Bandpass Filter

This bandpass filter can be mounted to the holder located on the excitation side of the solid sample block. The center wavelength is 250 nm, half bandwidth is 30 nm, with a 5 mm thickness and 25 mm cell size.

# Microsampling

used with all FP-8000 SeriesAll Modelsused only with FP-8200FP-8200used only with FP-8300FP-8300used only with FP-8500FP-8500used only with FP-8600 and FP-8700FP-8600/8700used only with Spectra Manager<sup>™</sup>PCpurge is standardPurge

## Microcell Jackets and Microcells

When sampling very small volumes, two microsampling accessories are available. The micro cell jacket and micro cell (FMH-857 and J/3-3.45/Q/3\*) is a 3x3 mm cell designed for sample volumes as small as 50  $\mu$ L. The FMH-802 and J/3-5.45/Q/5\* is a 5x5 mm quartz cell with 400  $\mu$ L volume with a stir bar and 500  $\mu$ L without.




FMH-857 with J/3-3.45/Q/3\*

FMH-802 with

J/3-5.45/Q/5\*

## **One-Drop Accessory**

The SAF-850/851 One-Drop accessory for the FP-8000 Series to measure micro-volume samples of protein and nucleic acids. The minimum sample volume is 5  $\mu$ L for the 1 mm pathlength cell and measurement only takes 15 seconds.

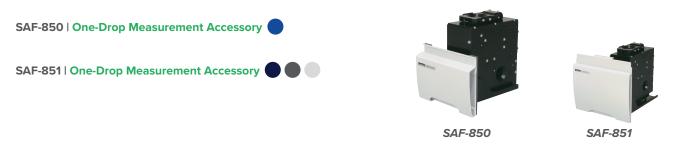


## **One-Drop Fluorescence Measurement**


The SAF-850 (FP-8200) or SAF-851 (FP-8300/8500/8600) One-Drop measurement accessory offers quantitative analysis or simple spectrum measurements requiring a minimum sample volume of 5  $\mu$ L. Without using a rectangular cell, easy and accurate measurements can be obtained with only one drop of sample from a pipette.



One-Drop Measurement System




Spectra of λ DNA labeled with PicoGreen (iRM type display example)



 $\begin{array}{c} \text{Calibration Curve of} \\ \lambda \text{ DNA labeled with PicoGreen} \end{array}$ 

# Integrating Spheres and Phosphorescence

Phosphorescence data can be obtained using a variety of measurement programs such as Spectra Measurement, Quantitative Calibration and Analysis, Fixed Wavelength Measurement, Time Course Measurement, and Phosphorescence Lifetime Measurement.

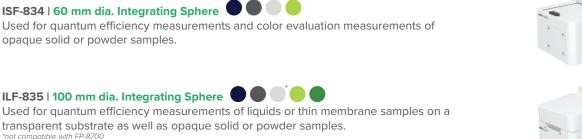

#### ILFC-847 | LN, Cooled 100 mm dia. Integrating Sphere

Used for quantum efficiency measurement of samples cooled with liquid nitrogen. It can also be used at ambient temperatures without liquid nitrogen. not compatible with FP-8700







#### Specifications

| Model Name                                  | ISF-834                      | ILF-835                      | ILFC-847   |
|---|------------------------------|------------------------------|--|
| Inner Diameter                              | 60 mm                        | 100 mm                       | 100 mm   |
| Minimum Sample Size                         | 20 (H) × 20 (W) × 0.5 (T) mm | 20 (H) x 10 (W) x 0.5 (T) mm | 20 (H) × 10 (W) × 0.5 (T) mm   |
| Maximum Sample Size                         | 60 (H) x 50 (W) x 25 (T) mm  | 30 (H) × 20 (W) × 6 (T) mm   | 30 (H) × 20 (W) × 6 (T) mm   |
| Cells                                       |                              |                              | 1,2 mm liquid cell, 3 mm powder cell, 10 mm rectangular cell, KBr plate sample holder, LPH-140, PPH-150, CPH-160 |
| Optional Spectral Correction<br>Accessories | ESC-842, ESC-843             |                              |  |



Cells for Integrating Spheres

- 1 mm liquid cell Path length:
- Path width:
- Sample volume:

2 mm liquid cell

Path length: Path width: Sample volume:

2 mm 10 mm 3 mm powder cell

19 (H) x 10 (W) x 3 (T) mm Cell size:

10 mm Rectangular Cell Holder

Used to mount a 10 x 10 mm rectangular cell inside the ILF-835/ILFC-847 integrating spheres.



1 mm


10 mm

2 μL

#### **KBr Plate Sample Holder**

400 μL

Used to sandwich a powder sample between two KBr plates (5 × 5 × 1 mm). This accessory can also be used for micro FTIR measurements.



| All Models   | used with all FP-8000 Series  |
|--------------|-------------------------------|
| FP-8200      | used only with FP-8200        |
| FP-8300      | used only with FP-8300        |
| FP-8500      | used only with FP-8500        |
| FP-8600/8700 | nly with FP-8600 and FP-8700  |
| PC           | ed only with Spectra Manager™ |
| Purge        | purge is standard             |
|              |                               |

#### **ACCESSORIES AND APPLICATIONS**

## PMU-830 | Liquid Nitrogen Cooling Unit

Used to measure samples cooled with liquid nitrogen.

#### Specifications

| Cooling Temperature | 77 K (-196°C)             |
|---------------------|---------------------------|
| Optional Cells      | LPH-140, PPH-150, CPH-160 |



LPH-140 | Phosphorescence Measurement Cell Kit for Liquid Sample PPH-150 | Phosphorescence Measurement Cell Kit for Powder Sample CPH-160 | Phosphorescence Measurement Cell Kit for Solid Sample



**PPH-150** 



Specifications

| LPH-140                           | PPH-150                              | CPH-160   |
|-----------------------------------|--------------------------------------|---|
| Tube Size: 5 mm O.D. x 178 mm     | Cell Size: $\phi$ 7 mm x 0.5 or 1 mm | Min Sample Size: 5 (H) x 5 (W) x 1 (T) mm or 1 mm |
| Tubing Material: Synthetic quartz |                                      | Max Sample Size: 18 (H) x 10 (W) x 3 (T) mm       |

LPH-140

used or

CPH-160

#### CSH-831 | Cryostat Holder Used with either the Optistat DN or DN-V by Oxford instruments. OBF-832 | Optical Fiber Unit 🔵 🔵 🔵 Used to measure a sample located outside Specifications the sample compartment using either a 1 or 2 m optical fiber probe. EFA-833 | Epi-Fluorescence Unit

Used to irradiate a sample facing downward on the top of the accessory and to measure the samples epifluorescence. The minimum incident beam size is  $1 \times 1.5$ mm with a 45° incident angle.



#### HPC-836 | High Temperature Powder Cell Unit


An internal heater provides temperature control for measuring the effects of temperature variation on the sample fluorescence intensity.

| Temp Control System   | Heating system   |
|-----------------------|--|
| Heat Radiation System | Water-cooled   |
| Temp Control Range    | Room temperature + 25 to 300°C<br>(cooled water temperature at 25°C) |
| Temp Stability        | ±1℃  |
| Standard Cell         | Powder cell A, φ 20 mm X 1 mm<br>Powder cell B, φ 20 mm x 0.5 mm     |



# Fluorescence Polarization Anisotropy


Fluorescence anisotropy occurs when a fluorophore emits different intensities of light dependent on the polarization angle of the incident light. Fluorescence anisotropy can be used to probe the structural flexibility of a fluorophore, which cannot be obtained by fluorescence spectroscopy alone.

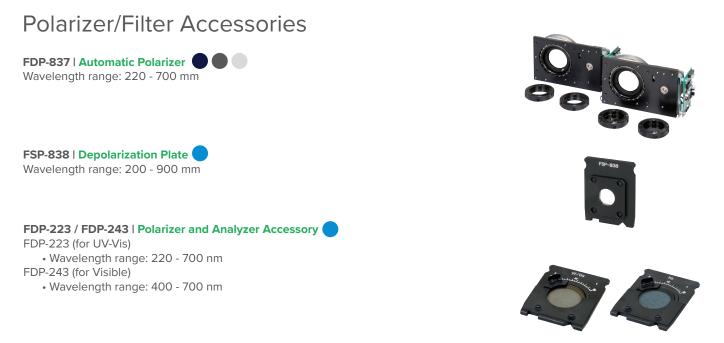

## Example of Anisotropy Measurement

A fluorescent dye (DPH) was added to a lipid bilayer and the degree of polarization was measured as a function of temperature, as well as the fluorescence intensity and anisotropy. The data obtained can be used to elucidate binding properties and phase transitions induced through vesicle interactions and the heat of temperature changes.



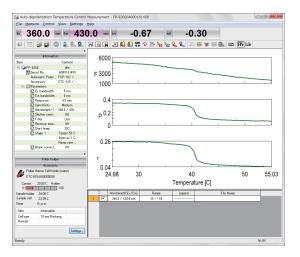


Measuring Degree of Polarization of Liposome

# Automated Titration and Stopped-Flow

## Automated Titration

The auto titrator is used to monitor changes in the fluorescence intensity as a function of pH, chemical denaturant, or exogenous ligands. Dual syringes are employed and are each fitted with a valve for automated refilling and flushing during extended runs and for maintaining a constant cell volume. In addition, the titration measurement program automatically corrects for concentration.



Automatic Titration Measurement Program Measurement Screen



#### Specifications

| Model:                     | ATS-826                   | ATS-827                    |  |  |  |
|----------------------------|---------------------------|----------------------------|--|--|--|
| Compatible Cells:          | Micro cell 5 x 5 mm, r    | ectangular cell 10 x 10 mm |  |  |  |
| Compatible Accessories:    | STR-811, ETC-814          | STR-812, EHC-813, ETC-815  |  |  |  |
| Number of Syringes:        | 2                         |                            |  |  |  |
| Syringe Volume Options:    | 1.0 mL (standard), 2.5 mL |                            |  |  |  |
| Injection Accuracy:        | Greater than 99%          |                            |  |  |  |
| Injection Reproducibility: | Less than 1%              |                            |  |  |  |
| Injection Pitch:           | 0.1% of syringe volume    |                            |  |  |  |



\*The PC control software is included as standard.

## Stopped-Flow

The Stopped-Flow accessory is used to rapidly mix two or more solutions to trigger a chemical reaction. The reaction kinetics are then followed by monitoring the change in the fluorescence intensity.

#### SFS-852/853/854/852T/853T/854T | Stopped-Flow Accessory

| ū |  |
|---|--|
|   |  |

SFS-852

| Model:                      | SFS-852   | SFS-853 | SFS-854 | SFS-852T                                | SFS-853T | SFS-854T |
|-----------------------------|---|---------|---------|---|----------|----------|
| Number of Syringes:         | 2   | 3       | 4       | 2                                       | 3        | 4        |
| Syringe Volume Options:     | 10 mL (standard), 1.0, 2.5, 5.0 mL                |         |         |   |          |          |
| Mixing Ratio:               | 1:1 to 1:20                                       |         |         |   |          |          |
| Dead Time:                  | 2.9 msec.   |         |         |   |          |          |
| Flow Rate:                  | 5 mL/sec. (10 mL syringe)                         |         |         |   |          |          |
| Temperature Control System: | - Heating/cooling system utilizing Peltier effect |         |         |   |          |          |
| Peltier Heat Radiation:     | – Water-cooled                                    |         |         |   |          |          |
| Temperature Setting Range:  |   | -       |         | Cell: 10 to 80°C<br>Syringe: 10 to 60°C |          |          |
| Temperature Accuracy:       |   | -       |         | ±0.5°C (cel)                            |          |          |
| Optional Accessory:         | 50 μL, 100 μL, 500 μL delay line                  |         |         |   |          |          |

\*The PC control software is included as standard.

# Autosampling

## Autosampling Systems

The autosampler system obtains automated measurement by combining an autosampler, syringe pump or sipper, and flow cell unit. Up to 192 liquid samples can be measured on all FP-8000 models, however, there are various rack options that can be used with either test tubes and/or vials. The system allows for automated scanning measurements at predetermined parameters using a flow cell. The PC control Spectra Manager<sup>™</sup> software is included as standard.



#### ASU-800 | Autosampler Unit

Optional sample racks (must be specified)

| Rack                                       | Compatible Test Tube and Vial                                      | Max No. of<br>Samples |
|--|--|-----------------------|
| SRA-811 15 mm O.D. Test Tube               | 15 mm O.D. test tube, 15 mm (O.D.) ×105 mm (H), 10 mL, 100 pcs/set | 100                   |
| SRA-812 13 mm O.D. Test Tube               | 13 mm O.D. test tube, 13 mm (O.D.) × 100 mm (H), 7 mL, 100 pcs/set | 100                   |
| SRA-813 12 mm O.D. Test Tube               | 12 mm O.D. test tube, 12 mm (O.D.) × 105 mm (H), 5 mL, 100 pcs/set | 150                   |
| ISRA-814 10 mm O.D. Test Tube              | 10 mm O.D. test tube, 10 mm (O.D.) × 90 mm (H), 3 mL, 100 pcs/set  | 150                   |
| SRA-818 Vial                               | Screw top vial, 2 mL, 500 pcs./set                                 | 120                   |
| SRA-816 Microplate                         | 96-well microplate, 250 μL   | 192                   |
| SPA-817 Constant Temperature<br>Microplate | 96-well amplification plate, 250 µL                                | 192                   |



**ASP-849** 

#### ASP-849 | Syringe Pump

Can be used in conjunction with ASU-800 and FSC-823/824 micro flow cell holder. The ASP-849 can be used with syringe volumes of 1.0. 2.5, 5.0, and 10.0 mL and has a reproducible volume delivery within  $\pm$ 1%.



| QFS-821   Vacuum Sipper<br>QFS-822   Vacuum Sipper<br>Specifications |                  |  |  |  |  |
|--|------------------|--|--|--|--|
| Cell Capacity  | 120 μL           |  |  |  |  |
| Cell Material  | Synthetic quartz |  |  |  |  |
| Tubing Material  | Teflon, SUS      |  |  |  |  |
| Carryover  | Less than 2%     |  |  |  |  |
| Min Sampl Requirement  | 700 μL           |  |  |  |  |

#### AWU-820 | Washing Unit

Optional washing unit for use with QFS-821/822 and SHP-819/820.



FSC-823

#### **Flow Cell Holders**

 FSC-823 | Micro Flow Cell Holder

 FSC-824 | Micro Flow Cell Holder

 15, 30, and 100 μL flow cell blocks are available.

SHP-819



15 uL

Synthetic quartz

Less than 2%

700 μL

PharMedTeflon, SUS

SHP-819 | Peristaltic Sipper SHP-820 | Peristaltic Sipper

Specifications

Cell Material

Carryover

Tubing Material


Min Sample Requirement

FSC-824

# Microplate Reader

## Microplate Reader

The FMP-825 Microplate reader can be used with the FP-8300 and FP-8500. Four standard measurements are available including Spectra Measurement, Quantitative Analysis, Time Course, and Fixed Wavelength. Quantitative Analysis can be used to create a calibration curve, as well as measure unknown samples in a single microplate while the Time Course Measurement software can be used to measure parallel kinetics for multiple samples.

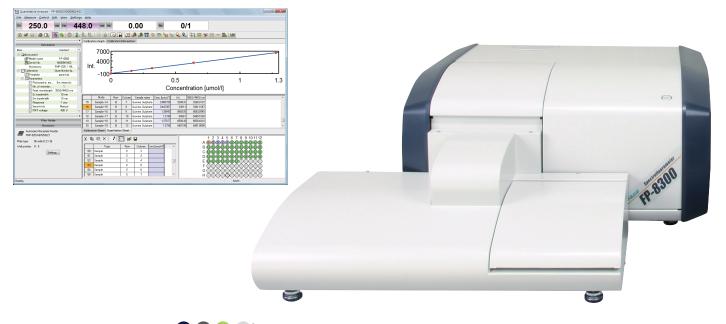

#### FMP-825 | Microplate Reader 🔵 🔵 🔵

| Specifications              |  |
|-----------------------------|--|
| Compatible Plate            | 96-well and 384-well black microplate for fluorescence (SBS standard), 1 pc. |
| Measurement Time            | 1 min./plate (96-wells, fixed wavelength measurement, specified condition)   |
| Min Sample Requirement      | 80 μL/well (96-well microplate)  |
| Photometric Reproducibility | ±3%  |
| Optional Accessories        | Constant temperature microplate holder                                       |
| Temperature Control System  | Heating system   |
| Temperature Control Range   | Room temperature +10 to 50°C   |

\*not compatible with FP-8700



els used with all FP-8000 Series

FP-8200 used only with FP-8200

FP-8300 used only with FP-8300

FP-8500 used only with FP-8500

<sup>0/8700</sup> used only with FP-8600 and FP-8700

used only with Spectra Manager™

Purge purge is standard

# Spectra Manager™ Software Suite

#### **Instrument Control**

Drivers are included to control each spectroscopy instrument and parameter dialogs allow easy editing of presaved parameter files. Data acquired from each instrument is automatically loaded into the analysis program to free up the PC and control software to acquire more data during post-acquisition processing. Each instrument driver also has its own dedicated application for instrument hardware diagnostics and validation.

#### **Flexible Display Features**

User-friendly features include overlay printing in colors and patterns, autoscale mode, and style and font, as well as customized toolbars.

#### **Data Processing and Spectral Analysis**

View and process several types of measurement data files (UV/Vis/NIR, FTIR, Fluorescence, CD) in a single window, using a full range of data processing functions. Features include arithmetic operations, derivatives, peak detection and processing, smoothing, and baseline correction.

#### **Report Publishing**


JASCO Canvas allows users to create layout templates of spectral data and results to meet individual reporting requirements.


#### **Macro Command Option**


This software can be used to develop user-designed application programs for individual experimental set-up and routine measurements, including instrument control, data acquisition, post-acquisition data processing and reporting.

#### Secure Access with Spectra Manager<sup>™</sup> CFR

Spectra Manager CFR provides secure access and compliance with 21 CFR Part II. System access requires a username and password, which are assigned by the Workgroup Manager. Individual levels determine the access to administrative tools that include instrument and analysis application installation, user and workgroup setup, security policies, as well as system and application history logs. Three levels of electronic signatures are required, including creation, review, and approval stages. An audit trail is assigned to every data file, recording any spectral data processing.

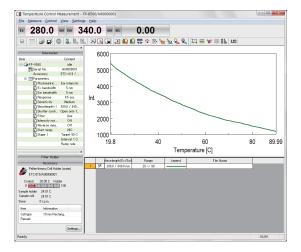

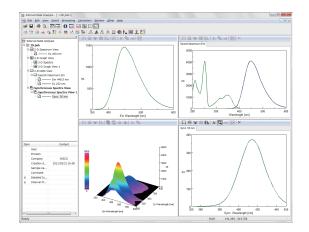

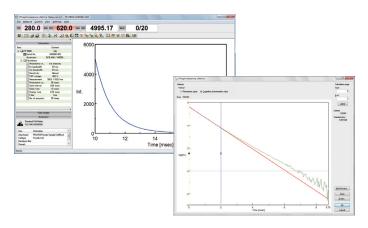



# A SINGLE PLATFORM FOR EVERY INSTRUMENT.

JASCO is the only manufacturer to develop a powerful, cross-platform 64-bit Windows software package for controlling a wide range of spectroscopic instrumentation. Spectra Manager<sup>™</sup> is a comprehensive lab companion for capturing and processing data, eliminating the need to learn multiple software programs and allowing data from more than one instrument to be analyzed and displayed together on the same platform.

# Standard Measurement Programs

#### **Spectra Measurement**

The FP-8000 series spectrofluorometer can measure five different types of spectra: emission, excitation, synchronous, single-beam emission and single-beam excitation in both fluorescence and phosphorescence\* modes.

\*Excludes FP-8200.

#### **Time Course Measurement**

The Time Course Measurement program is used for measuring temporal changes of fluorescence intensity at a fixed wavelength. Up to 100,000 hours (FP-8300/8500/8600) and 1,667 hours (FP-8200) of continuous measurements can be performed using a 60 minute and 60 second interval, respectively.

#### **Quantitative Analysis**

In the Quantitative Analysis software, optimal parameters from two photometric modes, emission and excitation, and three quantitation methods, no base (1 wavelength), one-point base (2 wavelengths) and two-point base (3 wavelengths) can be selected depending on the application. Other quantitative calibration curve methods such as log or spline functions are also available.

#### **Fixed Wavelength Measurement**

This program can be used to measure a sample's fluorescence or phosphorescence intensity at fixed excitation and emission wavelengths for up to four wavelengths.


#### **Phosphorescence Lifetime Measurement**


Measures changes in the phosphorescence of a sample briefly irradiated by the excitation source.


\*Excludes FP-8200.

#### **Interval Scan Measurement**

Measures up to three spectra (fluorescence, excitation, and synchronous) and displays the results as either 2D or 3D spectra, as well as contour or color-coded plots.

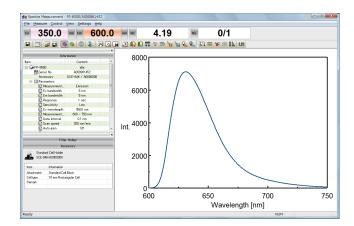

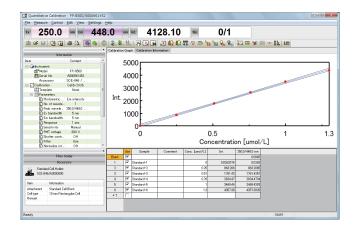

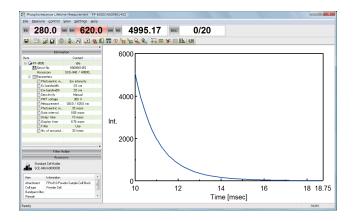

#### **Spectral Correction**

Allows users to easily compare measured spectral data from several instruments as well as determine the quantum yield efficiency. Corrected spectra can be obtained immediately after the measurement is completed. The FP-8200/8300 require optional jigs for spectral correction. A Rhodamine B ethylene glycol solution is also included as a standard and additional sources for correction can be obtained separately.

#### **Relative Quantum Yield**

All models in the FP-8000 Series include a relative quantum yield calculation program as standard.

#### **Absorbance Spectra Measurement**


Obtain the transmittance, absorbance, or reflectance spectrum by measuring the synchronous spectrum of a sample. The optional FUV-803 Absorbance measurement cell block is required for absorbance and transmittance measurements while reflectance measurements require an integrating sphere.


#### **3D Measurements**


Allows for the simultaneous display of several different sets of data, including 2D, 3D, and synchronous spectra. The 3D plots can be viewed in Contour, Color 3D, and Color-mapping.

#### Validation

The validation program includes instrument test procedures in compliance with JIS (K 0120 2005) and JAIMAS (0004-2005). This program provides six performance tests including wavelength accuracy, wavelength repeatability, resolution, stray light, sensitivity, and photometric stability. The test results and procedures can be saved and/or printed.

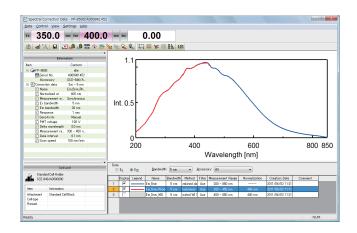

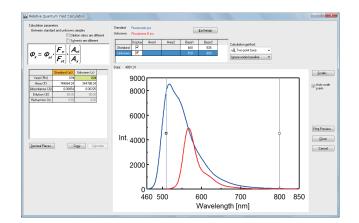

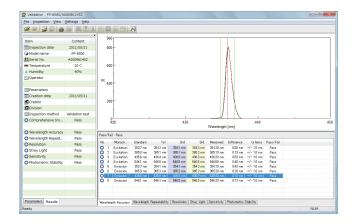

# **Optional Software**

Measurement Programs - From Data Acquisition to Data Processing and Analysis

#### FWTP-874 | Temperature Control Measurement

This application can be used to evaluate the melting temperatures of biological samples. The melting temperature,  $T_m$ , is calculated from the results of a time course measurement during a temperature change. The ETC-814/815 single position or PCT-818 Water-cooled Peltier thermostatted 4-position cell holders are required for use.

#### FWTS-872 | Temperature Interval Scan Measurement

This program is used to acquire excitation and emission spectra at a defined temperature interval with a temperature controlled accessory such as the ETC-814/815 single position or PCT-818 Water-cooled Peltier thermostatted 4-position cell holders.

#### VWKN-772 | Advanced Kinetics Analysis

This application program obtains a time course kinetic measurement and plots the data in various graphs, as well as calculates the maximum reaction velocity ( $V_{max}$ ), Michaelis-Menten constant ( $K_m$ ), and Hill constant (n). This program can be used with automated cell holders.

#### FWAP-875 | Fluorescence Polarization Measurement

The total fluorescence intensity (F), fluorescence anisotropy (r), and degree of polarization (P) can be measured using the FDP-837 automatic polarizer unit, providing auto-depolarization fixed wavelength measurements or auto-depolarization time course measurements.

#### FWQE-880 | Quantum Yield Calculation

Calculates the quantum yield of a sample with the use of an integrating sphere as well as the ESC-842 calibrated light source (WI).

\*Excludes the FP-8200.

#### FWTC-873 | Dual-Wavelength Time Course Measurement

Enables time course measurements of the ratio of fluorescence intensities at two different wavelengths for either the excitation or emission. The calcium concentration calculation function in the program can also calculate the change in concentration of an intracellular ion.

#### FWFC-878 | Fluorescent Object Color Measurement

Enables evaluation of fluorescent sample color (fluorescent objective color) using the ISF-834 60 mm diameter integrating sphere, ESC-842 calibrated light source (WI), or WRE-362 PMT. This program calculates the fluorescent sample color using a desired light source when the spectra of the various light sources are pre-registered. Spectral measurements are required in the range wider than 300 - 780 nm for excitation and 380 - 780 nm for emission.


\*Excludes the FP-8200.


#### FWLU-879 | Luminous Color Measurement


Obtains the luminescence or emission spectra of light emitting samples using either the ESC-842 Calibrated light source (WI) or the WRE-362 PMT for wavelength expansion. Data analysis includes a colored chromaticity diagram and calculation of the correlated color temperature and color rendering index.


#### FWMC-883 | Macro Command

Executes a sequence of pre-programmed operations automatically, including parameter setting, measurements, analysis and printing.









# iRM-1200 Intelligent Remote Module

The iRM-1200 intelligent remote module incorporates a color LCD touch screen to easily access all functions, which can be used for both the FP-8200 and FP-8300. The iRM-1200 conveniently guides the operator through routines encompassing data acquisition to data processing. The obtained data can be automatically printed to USB PictBridge printers, or saved to a CF memory card for further processing on a PC.



Easy Data Transfer to a PC



Touch-Sensitive Screen



iRM-1200

- High quality color LCD display
- Operation using Touch Pen
- Enhanced quantitative analysis
  - Equipped with instrument validation software
- Print to a USB printer

### Standard Programs for the iRM-1200

Spectra Measurement Time Course Measurement Quantitative Analysis Fixed Wavelength Measurement Phosphorescence Lifetime Measurement Interval Scan Measurement Spectral Correction Relative Quantum Yield Absorbance Spectra Measurement 3D Measurements Validation

#### Optional Programs for the iRM-1200

FRTC-891 | Dual-Wavelength Time Course Measurement FRTP-892 | Temperature Control Measurement FRKN-893 | Advanced Kinetics Analysis FRAP-894 | Fluorescence Polarization Measurement FRMC-895 | Macro Command

| Load Parameters |
|-----------------|
|                 |
| Load Parameters |
| a Measurement 💌 |
|                 |
|                 |

#### **IQ Accessory and IQ Start**

User-friendly features include the IQ Accessory function for automatic accessory recognition and IQ Start for immediate start of pre-registered programs when conducting routine measurements.

#### Validation and Accessory Kits





#### ESC-842 | Calibrated WI Light Source

The ESC-842 is used for spectral correction of the emission optical system from 300 - 1010 nm.

#### ESC-843 | Calibrated D<sub>2</sub> Light Source

The ESC-843 is used for spectral correction of the emission optical system from 200 - 400 nm.



#### SID-844 | Calibrated Detector 🔵 🛑

The SID-844 is used for spectral correction of the excitation optics from 200 - 900 nm.



#### VDK-840 | Validation Kit 1

The VDK-840 is used for spectral correction of the excitation optics and for the stray light instrument validation test from 200 - 600 nm.



#### VDK-841 | Validation Kit 2

The VDK-841 consists of correction filters for the stray light instrument validation test.





\*The expanded wavelength range is described in the specification sheet.



All Models used with all FP-8000 Series FP-8200 used only with FP-8200 FP-8300 used only with FP-8300 FP-8500 used only with FP-8500 <sup>600/8700</sup> used only with FP-8600 and FP-8700 used only with Spectra Manager™ Purge purge is standard

# **Specifications**

| Model   |            | FP-8200  | FP-8300  | FP-8500  | FP-8600   | FP-8700                                |  |  |
|---|------------|--|--|--|---|--|--|--|
| Light Source                                      |            |  | Xel  | amp with shielded lamp hous  | e, 150 W  |  |  |  |
| Light Source (for Validation)                     | )          |  | Integrated, selectable low pressure mercury lamp |  |   |  |  |  |
| Photometric System                                |            | Ratio-photometer system using monochromatic light to monitor the intensity output of the Xe lamp |  |  |   |  |  |  |
| Monochromator                                     |            |  | Holographi                                       | c concave grating in modified  | Rowland mount   |  |  |  |
| Wavelength Range                                  | Ex         |  |  |  | Zero order, 200 - 850 nm  | Zero order,<br>200 - 850 nm            |  |  |
| (Standard)  | Em         |  | Zero order, 200 - 750                            | nm   | Zero order, 200 - 1010 nm   | Zero order,<br>300 - 1400 nm           |  |  |
| Wavelength Range (Option                          | al)        | Zero order, 20   | 0 - 900 nm                                       | Zero order, 200 - 850 nm   | N/A   | option 1700nm                          |  |  |
| Automatic Cut-Off Filter for<br>Diffraction Light | High-Order | Option   |  | Standard   |   | Standard                               |  |  |
| Sensitivity (RMS)*                                |            | 4,500:1  | 8,000:1  | 8,500:1  | 3,500:1   | 1400 nm - 8,000:1<br>1700 nm - 1,000:1 |  |  |
|   | Ex         |  |  |  | 1.0 nm (at 54   | 6.1 nm)                                |  |  |
| Resolution  | Em         | 2.5 nm (at 546.1 nm)   | 1.0 nn   | n (at 546.1 nm)  | 2.0 nm (at 54   | 6.1 nm)                                |  |  |
| 5   | Ex         | 0.5.5.40.00  | 4 0 5 5 40 00                                    |  | 1, 2.5, 5, 10,<br>L10 nn  |  |  |  |
| Band Width  | Em         | 2.5, 5, 10, 20 nm  | 1, 2.5, 5, 10, 20 nm                             | 1, 2.5, 5, 10, 20, L5, L10 nm  | 2, 5, 10, 20, 4<br>L20 nr   |  |  |  |
| Wavelength Accuracy                               | Ex         | 12.0   | 14.5   | 110  | ±1.0 nr   | n                                      |  |  |
|   | Em         | ±2.0 nm  | ±1.5 nm  | ±1.0 nm  | ±2.0 ni   | n                                      |  |  |
|   | Ex         | -15 nm   | ±1 nm  | ±0.3 nm  | ±0.3 nr   | n                                      |  |  |
| Wavelength Repeatability                          | Em         | ±1.5 nm  |  |  | ±0.6 nr   | n                                      |  |  |
| Wavelength Scan Speed                             | Ex         |  | °  | 10, 20, 50, 100, 200, 500,<br>1,000, 2,000, 5,000,<br>10,000, 20,000,<br>60,000 nm/min | 10, 20, 50, 100, 200, 500,<br>10,000, 20,000, 60  |  |  |  |
|   | Em         | 20, 50, 100, 200, 500, 1<br>10,000, 20,00  |  |  | 20, 50, 100, 200, 500, 1,<br>10,000, 20,000, 60,000   |  |  |  |
|   | Ex         |  |  | 60,000 nn  | ı/min   |  |  |  |
| Slew Speed Em                                     |            | 30,000 nm/min  |  | 60,000 nm/min  |   | n/min                                  |  |  |
| Response  |            | 20, 50, 100, 200,<br>500 msec, 1, 2, 4, 8 sec  |  | 10, 20, 50, 100, 200, 5  | 500 msec, 1, 2, 4, 8 sec  |  |  |  |
| Detector  |            | Ex: Silicon photodiode, Em: PMT Ex: Silicon PD, E<br>LN2 Cooled PM                               |  |  |   |  |  |  |
| Photometric Range                                 |            | -10,000 - 10,000   |  |  |   |  |  |  |
| Sensitivity Selection                             |            | High, Medium, Low, Very Low, Manual, Auto SCS  |  |  |   |  |  |  |
| Auto Gain   |            |  |  | Standard   |   |  |  |  |
| Shutter Function                                  |            |  |  | Standard (Automatic contro   | ol)   |  |  |  |
| Sample Illuminating System                        | 1          |  |  | Horizontal illumination  |   |  |  |  |
| Sample Compartment                                |            |  | 10 mm r  | ectangular cell holder, nitroge  | n purgeable   |  |  |  |
| Recognition of IQ Accessor                        | У          |  |  | Standard   |   |  |  |  |
| Start Button                                      |            |  |  | Standard   |   |  |  |  |
| Analog Output                                     |            |  |  | Standard   |   |  |  |  |
| Instrument Communication                          |            |  |  | USB 2.0  |   |  |  |  |
| Control and Data Processing                       |            | Spectra Manage   | Spectra Manager™/CFR, iRM                        |  |   |  |  |  |
| Spectral Correction                               |            | Optic  | Option (S  |  | Standard<br>(Spectral correction using a Rhodamine B ethylene glycol solution is standa<br>other jigs for spectral correction are available separately as options.) |  |  |  |
| Dimensions  |            | 490 (W) x 545 (D) x<br>270 (H) mm  | 520 (W) x 545 (D) x<br>270 (H) mm                | 570 (W) x 545 (I   | D) x 270 (H) mm   | 895 (W) x 807 (D) x<br>270 (H) mm      |  |  |
| Weight  |            | 33.6 kg  | 36 kg  | 39   | kg  | 40Kg                                   |  |  |
| Power Requirement                                 |            | 270VA  |  |  |   |  |  |  |
| Installation Environment                          |            |  | Temper   | ature: 15 to 35°C, Humidity: Le  | ss than 85%   |  |  |  |

\* Typical specification.



#### JASCO INTERNATIONAL CO., LTD.

11-10, Myojin-cho 1-chome, Hachio<sup>j</sup>i, Tokyo 192-0046, Japan Tel: +81-42-649-3247 Fax: +81-42-649-3518 http://www.jascoint.co.jp/english/ Australia, China, Hong Kong, India, Indonesia, Japan, Korea, Malaysia, New Zealand, Pakistan, Philippines, Russia, Singapore, Taiwan, Thailand

#### JASCO, INCORPORATED

28600 Mary's Court, Easton, Maryland 21601, U.S.A. Tel: +1-410-822-1220 Fax: +1-410-822-7526 Web: www.jascoinc.com Argentina, Bolivia, Brazil, Canada, Chile, Colombia, Costa Rica, Guatemala, Mexico, Paraguay, Peru, Puerto Rico, United States of America, Uruguay, Venezuela

#### JASCO EUROPE S.R.L.

Via Luigi Cadorna 1, 23894 Cremella (LC), Italy Tel: +39-039-9215811 Fax: +39-039-9215835 Web: www.jascoeurope.com JASCO Deutschland www.jasco.de | JASCO UK www.jasco.co.uk | JASCO France www.jasco.fr JASCO Benelux www.jasco.nl | JASCO Spain www.jasco-spain.com

Algeria, Austria, Belgium, Cyprus, Denmark, Egypt, Finland, France, Germany, Greece, Hungary, Iran, Iraq, Israel, Italy, Jordan, Kuwait, Lebanon, Luxembourg, Morocco, Netherlands, Norway, Poland, Portugal, Romania, Saudi Arabia, South Africa, Spain, Sweden Switzerland, Tunisia, Turkey, United Arab Emirates, United Kingdom, Yemen

